


TCVGH Temperature log

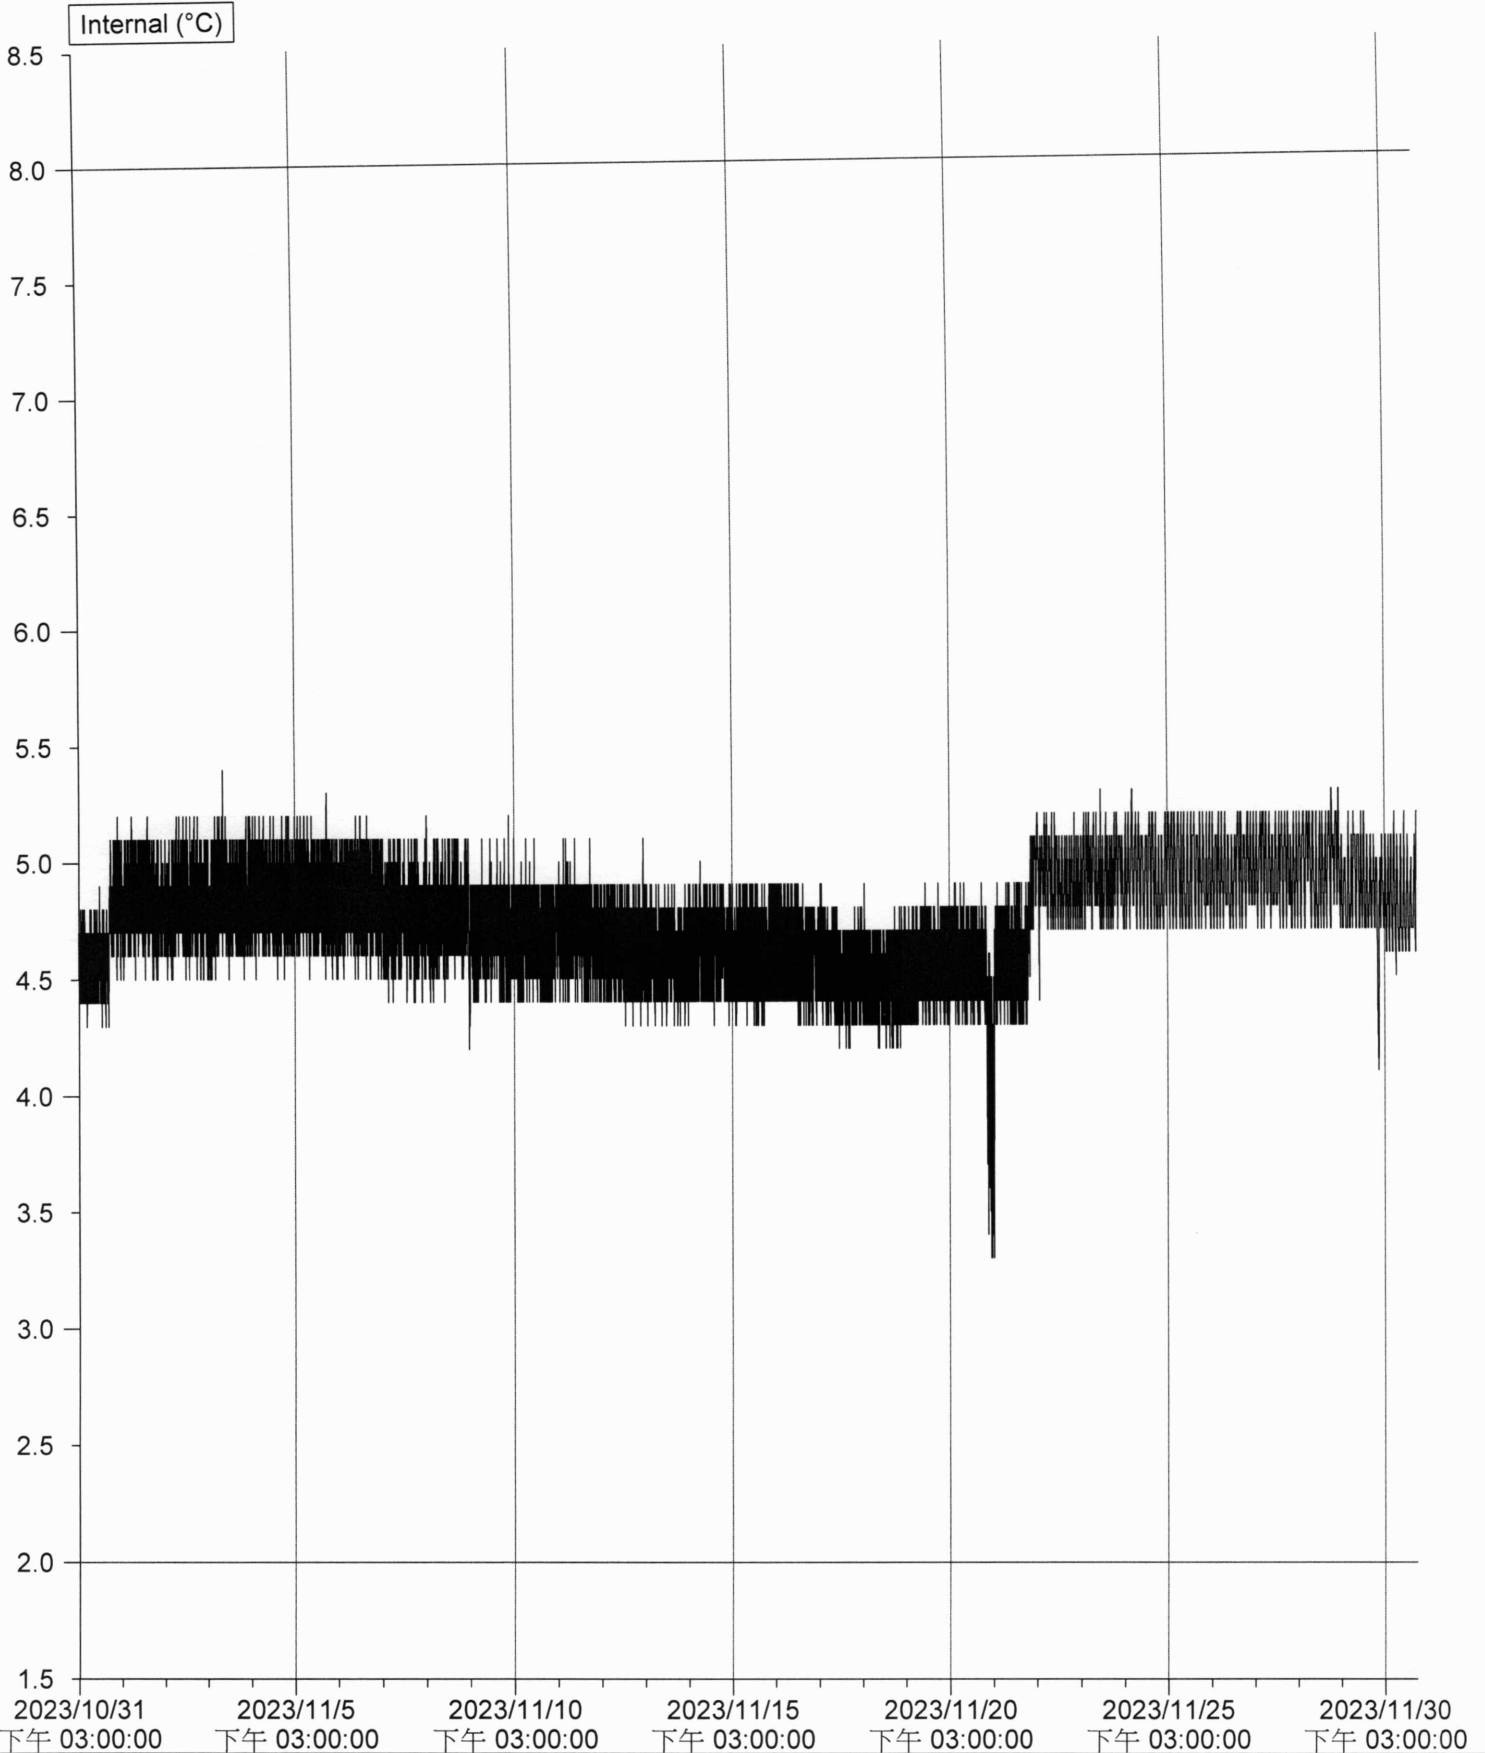

2023/10/31 下午 03:00:00 2023/11/5 下午 03:00:00 2023/11/10 下午 03:00:00 2023/11/15 下午 03:00:00 2023/11/20 下午 03:00:00 2023/11/25 下午 03:00:00 2023/11/30 下午 03:00:00

Sensor Name	Internal
Legend	
Description	PHCL-C005
Serial Number	1803-0051
Product Code	EI-IN-D-32-L
Start	2023/10/31 下午 03:00:00
Finish	2023/12/1 上午 08:30:00
Sensor Range	-40.5 to 70.4 °C
Specification	2.0 to 8.0 °C
Average	4.8 °C
Highest	5.4 °C
Lowest	3.3 °C

yuwenwang
01 Dec 2023