


# TCVGH Temperature Log

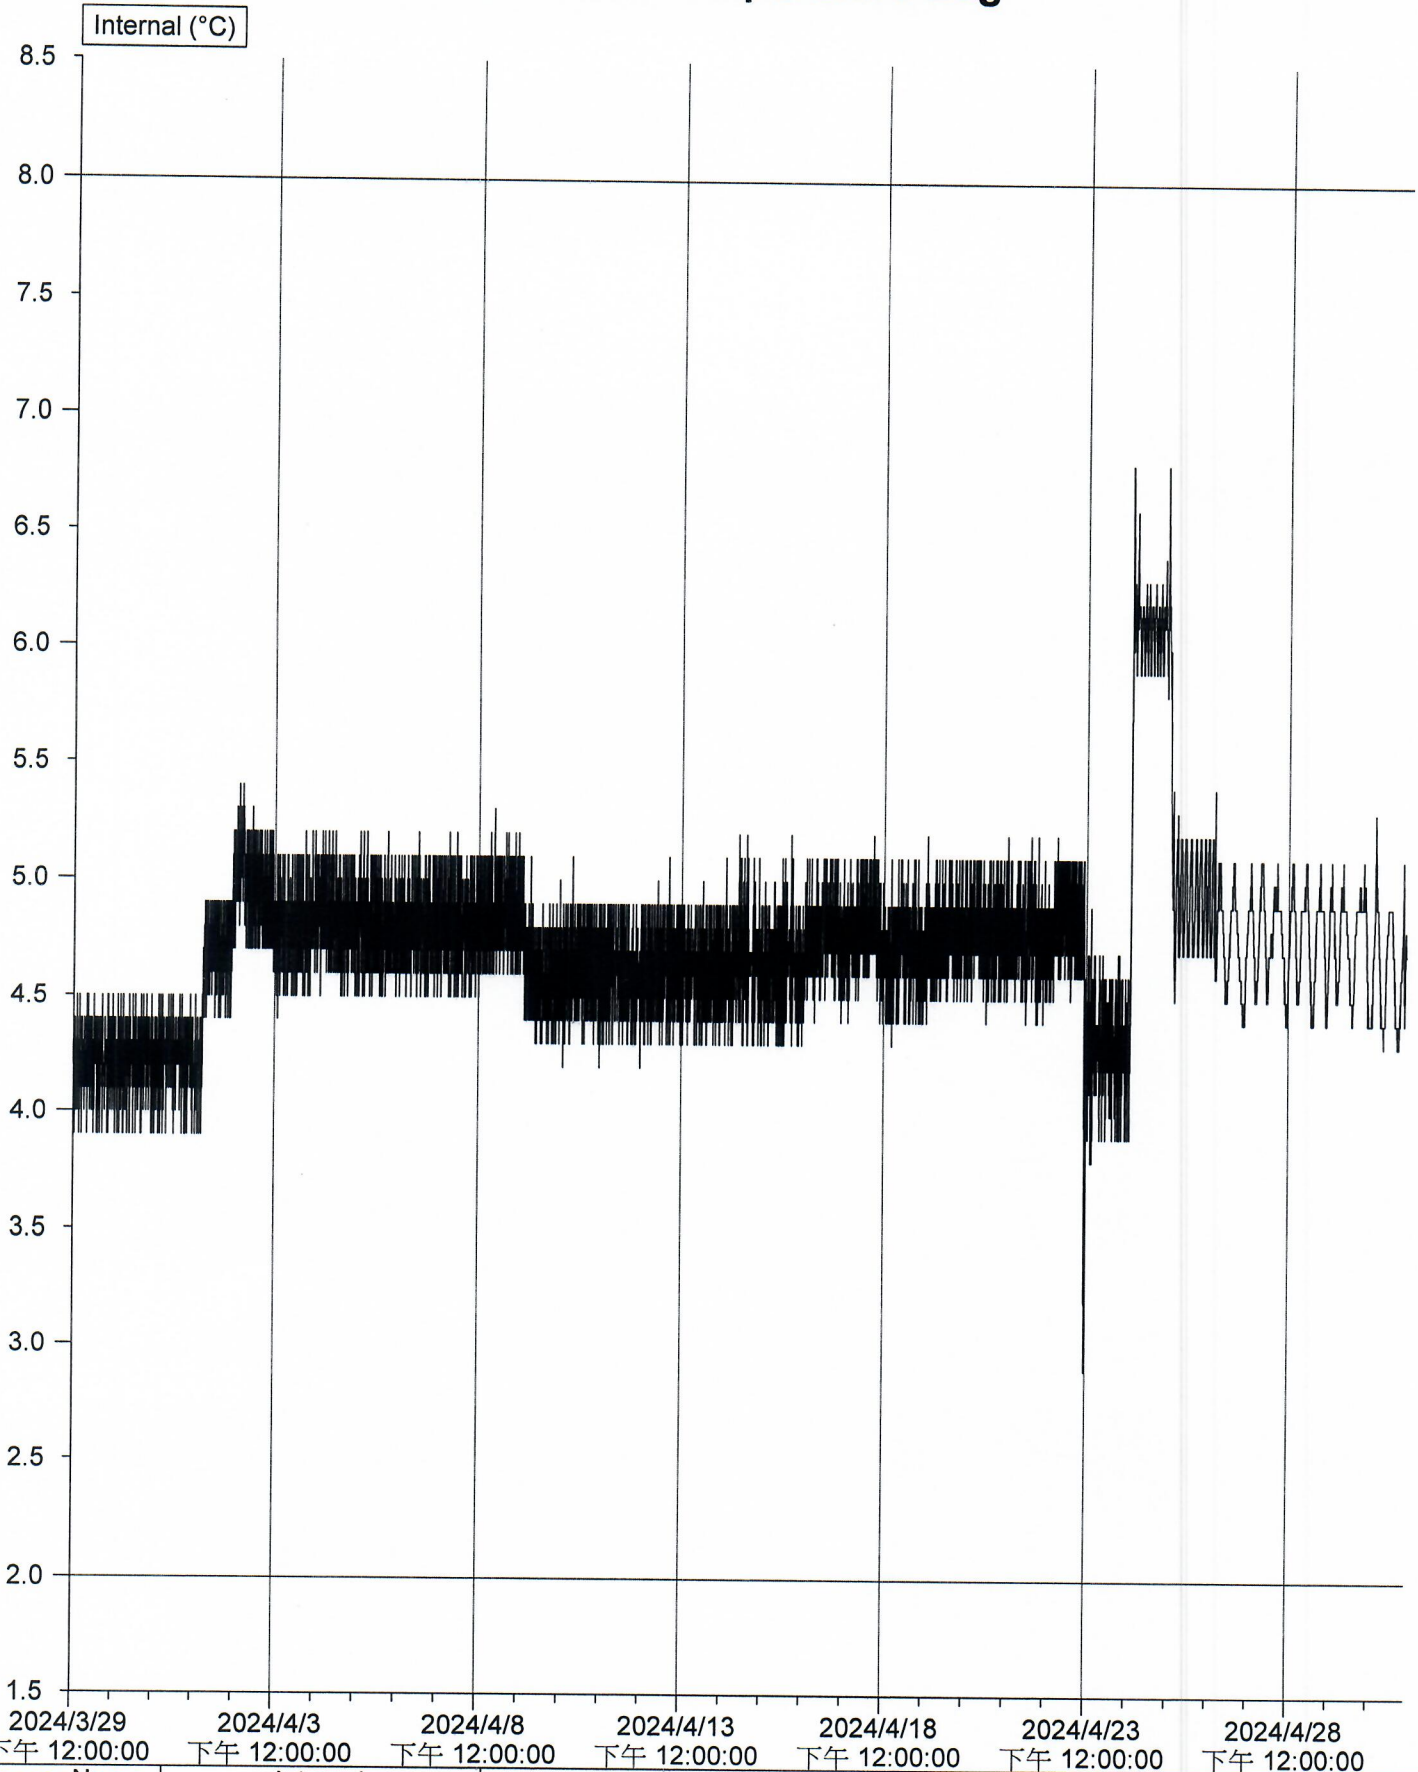

Sensor Name	Internal
Legend	
Description	PHCL-C005
Serial Number	1715-0115
Product Code	EI-IN-D-32-L
Start	2024/3/29 下午 12:00:00
Finish	2024/5/1 上午 10:20:00
Sensor Range	-40.5 to 70.4 °C
Specification	2.0 to 8.0 °C
Average	4.7 °C
Highest	6.8 °C
Lowest	2.9 °C

Yuchen Su  
01 May 2024

The refrigeration equipment PHCL-C005 is being retired.  
The Continuous temperature recorder and Investigation products have been transferred to PHCL-C015 on 29 Apr 2024.